
Combination Unidirectional Brachytherapy and SRS in the Treatment of Thoracic Spine Metastasis: A Cadaveric Study and Model


Introduction

- Brachytherapy has become an increasingly important treatment modality for a variety of cancers.¹
- However, considerable hesitance is required when implementing near neural structures such as the spinal cord and nerve roots.²
- Tumor recurrence often occurs in the posterior vertebral body and pedicle due to underdosing near these critical structures.
- Development of a brachytherapy device that is anisotropic, beta emitting, planar, palladium-103, low-dose rate, device that utilizes gold shielding to attenuate directional dose.²
- Here, we examine the feasibility of using this device in the thoracic spine.

Methods

- The membrane-like brachytherapy device was placed anterior to the spinal cord following exposure.
- The device was cut to fit the area and secured using 4 mm CMF screws. • An absorbable hemostatic agent (Surgicel Nu-Knit) was placed between the spinal
- cord and the device.
- The cadaveric specimen was subjected to XR, CT, and MRI imaging. • Dosimetry and radiation planning models were created using Eclipse and MIM software.

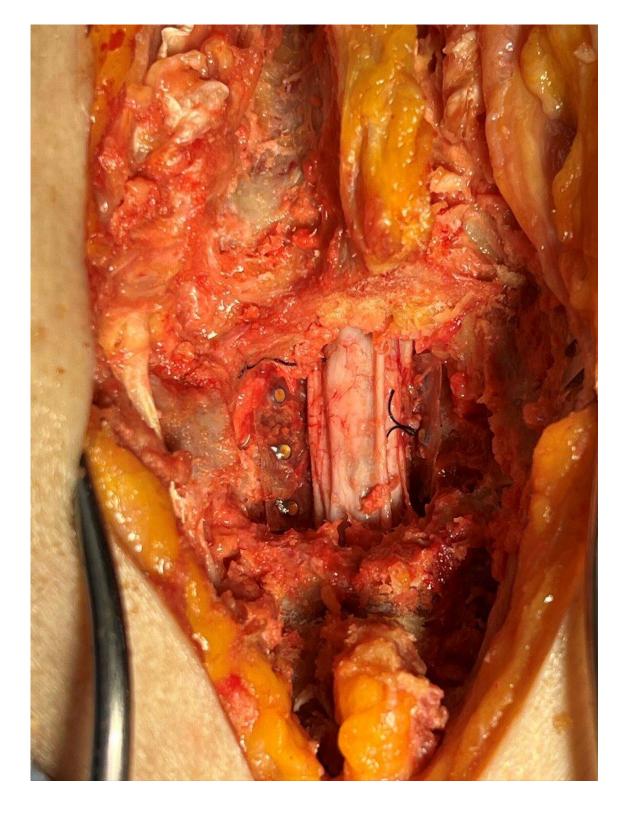

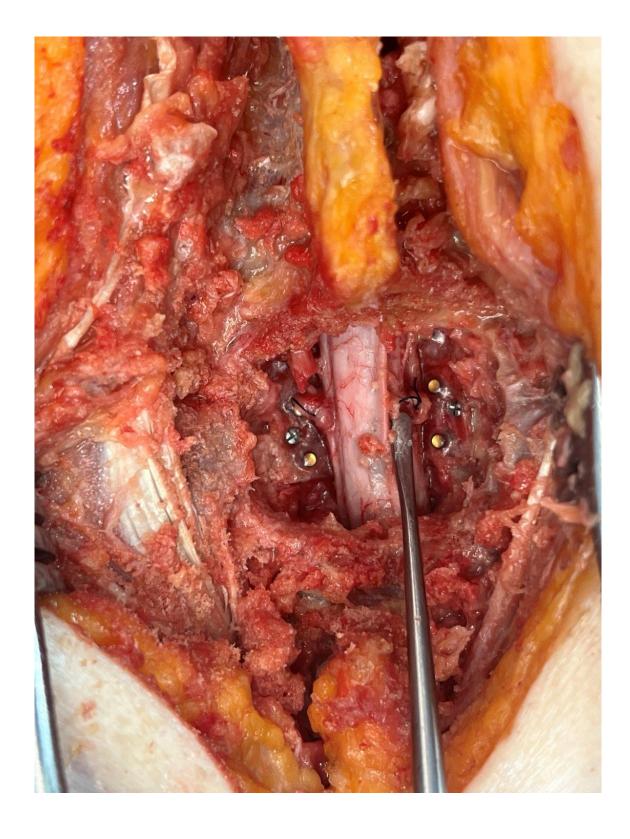


Nathan Ritchey, BS., Seth Wilson, BS, Joshua Weinberg, MD., Joshua Palmer, MD., Vikram Chakravarthy, MD.

Department of Neurological Surgery, Ohio State University Medical Center



- subsequent fluoroscopic imaging.
- posterior vertebral body.
- voxel (0.03 cc) = 9.2 Gy.
- anterior and middle vertebral body.
- coverage of the vertebral body.

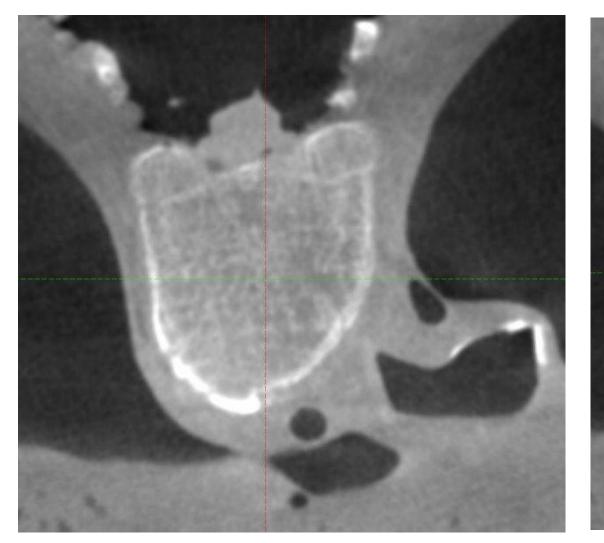



Surgical implementation of this device is feasible. The device demonstrated the ability to provide appropriate therapeutic doses to the vertebral body while sparing the spinal cord. Combined with adjuvant SRS, these techniques demonstrated complete therapeutic dose coverage and may provide improved local control. This is a limited cadaveric study with an n = 1. The goal of this study was to demonstrate the surgical feasibility of utilizing anisotropic brachytherapy in the spine. This novel approach shows promise and merits further evaluation.

• Device placement was achieved in the thoracic spine and confirmed through

Results

• The hemostatic spacer introduced a 1 mm clearance between the cord and device creating a notable drop off in dose delivered to the spinal cord.


• The device demonstrated a clear anisotropic dose distribution targeting the


• 12 sources were implanted with an observed 5.95 mCi per source.


• There was a total of 47 Gy 5 mm into the vertebral body with a cord max


Radiation planning contoured the brachytherapy dose distribution in the

• The combination brachytherapy and SRS approach demonstrated complete

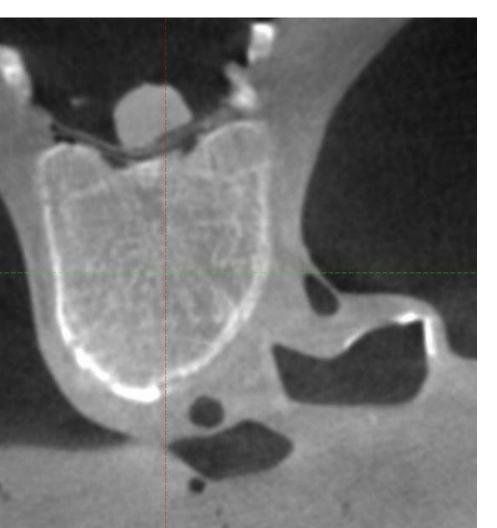

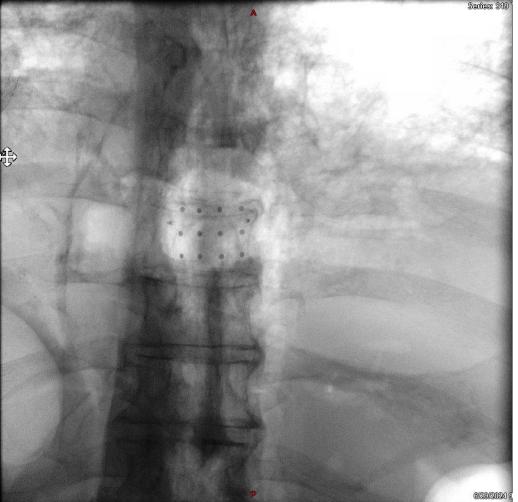

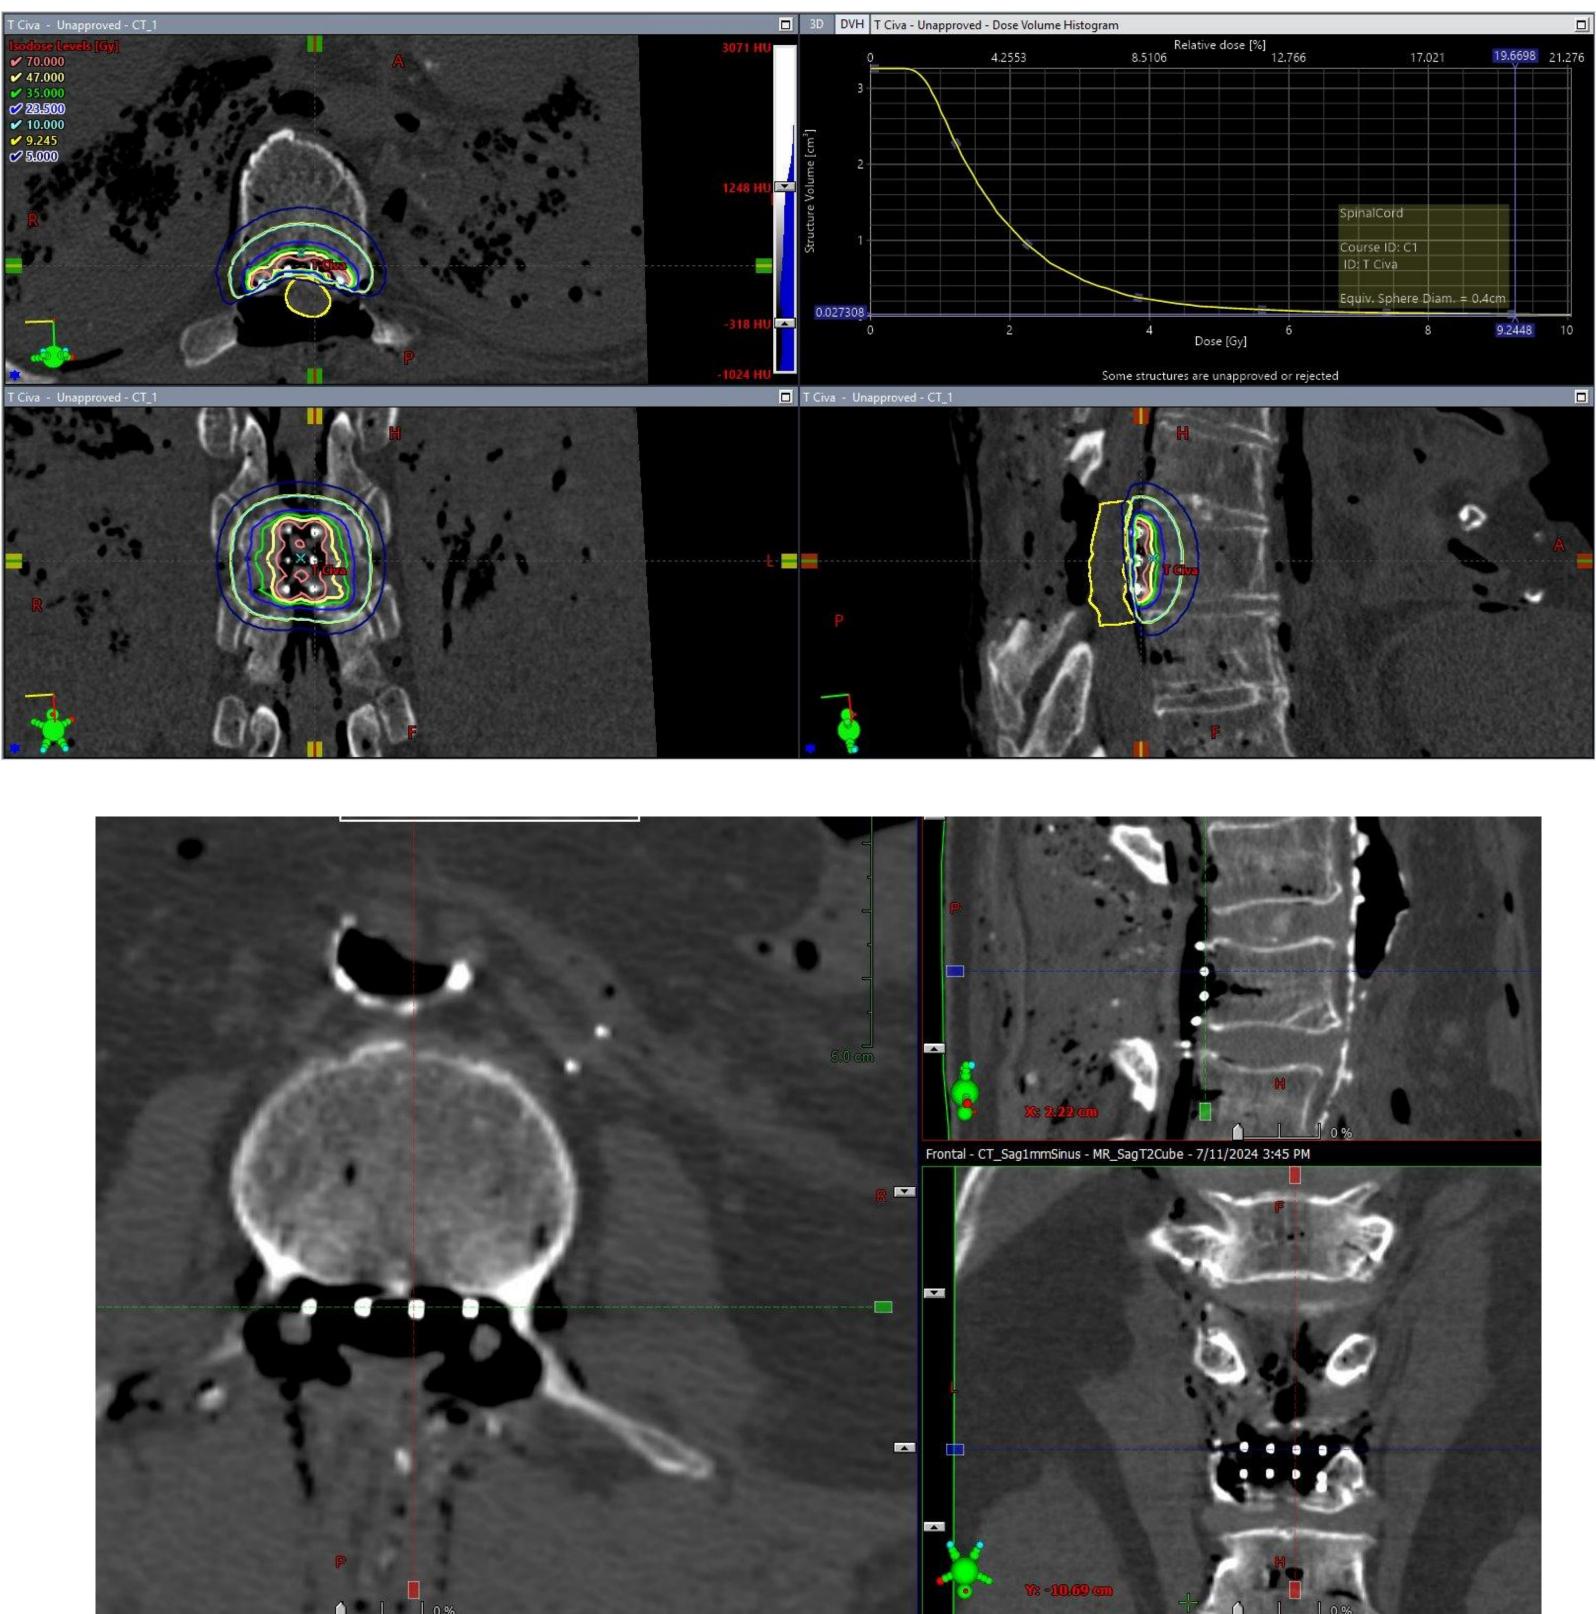

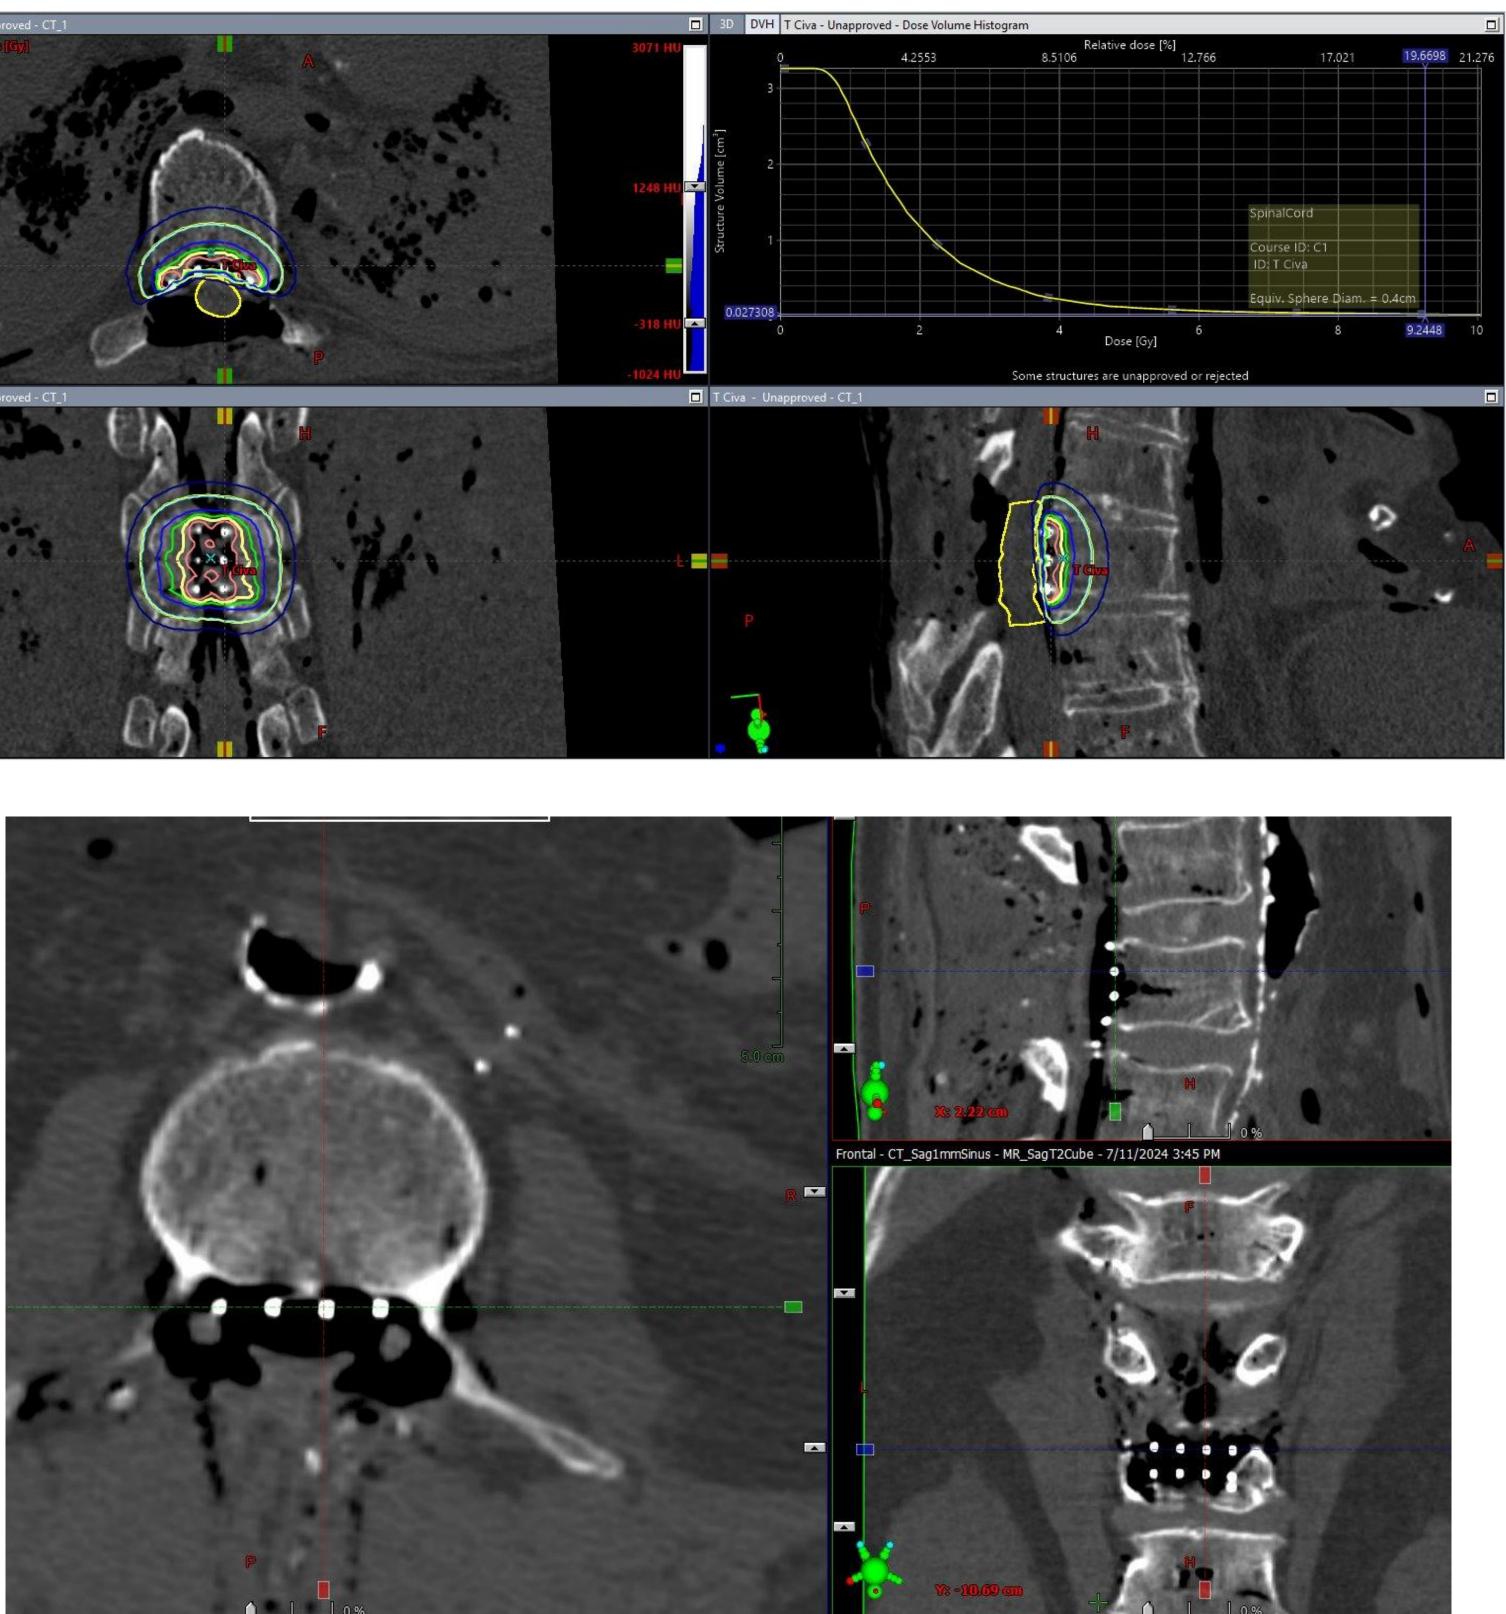

Conclusions, Limitations and Further Directions





The Ohio State University

COLLEGE OF MEDICINE

References

1. Mao G, Theodore N. Spinal brachytherapy. Neuro-Oncol. 2022;24(Supplement_6):S62-S68. doi:10.1093/neuonc/noac094

2. Seneviratne D, McLaughlin C, Todor D, Kaplan B, Fields EC. The CivaSheet: The new frontier of intraoperative radiation therapy or a pricier alternative to LDR brachytherapy? Adv Radiat Oncol. 2018;3(1):87-91. doi:10.1016/j.adro.2017.10.005